

Designed experiment optimizes method for removing endocrine disrupters

An endocrine disrupting chemical (EDC) is a synthetic chemical that, when absorbed into the body, either mimics or blocks hormones and disrupts the body's normal functions. EDCs can pass through wastewater treatment systems that are not currently designed to remove them.

A team of researchers recently performed a designed experiment to evaluate potential methods for removing three common endocrine disrupters. The researchers treated solutions containing the EDCs nonlyphenol (NP), bisphenol A (BPA) and triclosan (TCS) with an enzyme preparation from the white rot fungus *Coriopsis polyzona*.

"We used a designed experiment to optimize the temperature and pH at which the removal levels were the highest," said J. Peter Jones, Professor of the Department of Chemical Engineering, University of Sherbrooke, Québec. "The optimized conditions that we developed with the designed experiment removed 100% of the NP and BPA and 65% of the TCS in four hours."

Potential risk posed by EDCs

The endocrine system is a complex network of glands and hormones including the pituitary, thyroid, adrenal, thymus, pancreas, ovaries and testes. The endocrine glands release precise amounts of hormones into the bloodstream that serve as chemical messengers by controlling many bodily functions, including growth, development and maturation, as well as the way various organs operate. Examples of hormones include insulin which controls blood glucose, and estrogen and testosterone which affect female and male reproductive functions respectively.

Endocrine disrupters can reduce the production of hormones in, or affect the release of hormones from, endocrine glands. They also mimic or counteract the action of hormones in target tissues and speed up the metabolism of hormones, reducing their action. Previous

research has established that exposure to endocrine disrupters during early development may cause permanent harmful effects. Whether EDCs can have negative effects at the low levels at which such compounds are currently found in the environment has not been conclusively proven or disproven.

NP, BPA and TCS are EDCs that are frequently detected in waters downstream of wastewater treatment plants. NP comes from biodegradation in STP



of nonlyphenol ethoxylates which are mainly used as non-ionic surfactants in domestic and industrial applications. BPA is used as a raw material for the production of polycarbonates and epoxy resins. TCS is an antimicrobial agent that has been incorporated into personal care products such as toothpaste, deodorant sticks and soaps. Research has demonstrated that NP and BPA can bind to estrogen receptors, interfering with the action of estrogen while TCS can interact with thyroid hormones.

Recently, there has been a considerable amount of interest in white rot fungi (WRF) as a means of removing EDCs from the wastewater stream.

White rot fungus produces oxidative enzymes such as laccase, lignin, and manganese peroxidase that are relatively nonspecific biocatalysts. However, no studies prior to the current one have addressed the potential mechanism of elimination nor has there been a precise determination of the byproducts formed during enzymatic treatment.

Study designed to advance EDC removal methods

The two goals of this study were to evaluate the effectiveness of the removal of NP, BPA and TCS with WRF enzymes and to assess the transformation mechanisms by identifying the metabolites that were produced. The researchers also wanted to be sure that the elimination of the EDCs did not produce metabolites with estrogenic activity.

The researchers were well aware that the effectiveness of the removal of the EDCs could be affected by factors such as temperature and pH. This meant that accurate assessment of the effectiveness of the enzymes in removing EDCs required determining the effect of these factors and evaluating EDC removal with the factors optimized. The conventional approach to optimizing the factors would be to run a series of experiments while varying a single factor. The problem with this approach is that it does not detect interactions between factors or second order effects.

As a result, the researchers decided to use the design of experiments (DOE) method that varies the values of all variables in parallel so it uncovers not just the main effects of each variable but also the interactions between the variables. This approach makes it possible to identify the optimal values for all variables in combination. It also requires far fewer experimental runs than the one-factor-at-a-time (OFAT) approach.

"Designing experiments and analyzing the results using DOE can be time-consuming and error-prone when manual methods are used," Jones said.

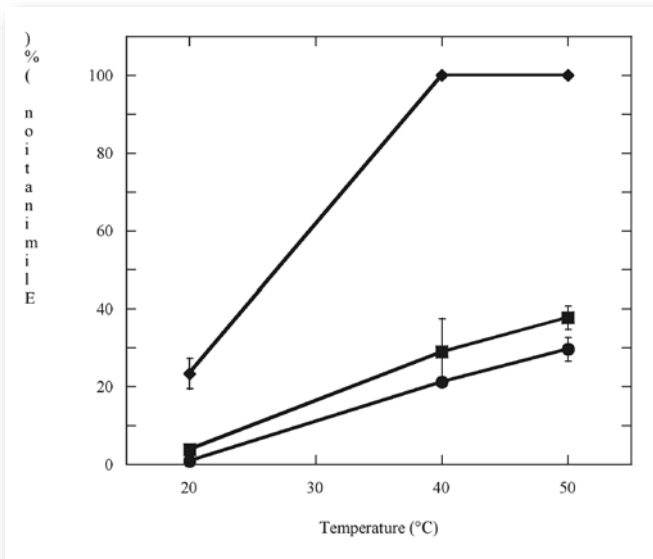


Fig 1. Effect of temperature and (■) pH 3, (●) pH 4 and (▲) pH 5 on the degradation of BPA after a 4-hour treatment with 10 U/l of laccase of *C. polyzona*.

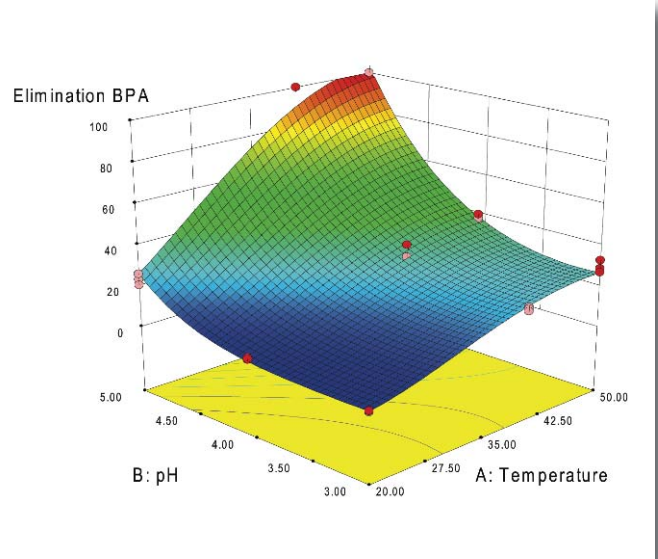


Fig 2. 3D graph view of the effect of temperature and pH on the degradation of BPA.

“General purpose statistical tools can do the job but tend to be unintuitive and limited in their choice of experimental designs and results analysis techniques. We used Design-Expert® DOE software from Stat-Ease, Inc., Minneapolis,

because it is very easy to use, yet provides very powerful capabilities including a wide range of experimental designs and powerful statistical methods to analyze the results.”

The researchers decided to look at

the following factors:

A) Temperature (20°C vs. 40°C vs. 50°C)

B) pH (3 vs. 4 vs. 5)

Design-Expert software generated a

continued overleaf...



**Tough, High Quality Pumps
Nationwide Dealer Network
Superior Service**

Claessen Pumps

Servicing The Canadian Industry Since 1976

Distributors of :

**POWER
PRIME
PUMPS**

GRINDEX

Phone: 705-431-8585

Fax: 705-431-2772

For more information please contact us or
visit our web site at www.claessenpumps.com

full-factorial experiment with nine runs for each substance to be removed. Each combination was replicated three times in a randomized run plan. The researchers mixed 5 mg/l of each NP, BPA or TCS, 5 U/1 catalase from *Aspergillus niger*, crude enzyme preparation from *Corioloropsis polyzona*, citric

acid/di-sodium hydrogen phosphate buffer, and 1% v/v methanol. NP, BPA and TCS were extracted from the mixture and analyzed on a high performance liquid chromatography system. The estrogenic activity of the treated system was compared to the system before treatment. Mass spectroscopy was used to identify high molecular weight metabolites. The results of the experiment were entered into Design-Expert and the software analyzed the statistical results.

DOE results identify optimal EDC removal conditions

A statistical analysis of variance (ANOVA) of the model highlights the significant impact of temperature and pH on the enzymatic transformation of NP, BPA and TCS. This analysis was used to determine the best conditions for enzymatic transformation of the three EDCs. The results showed that 50°C was the best temperature for the removal of NP and TCS, while the results for 40°C and 50°C were not significantly different in the case of BPA. A pH of 5 gave the best results for all three compounds studied. These results can be explained by the higher stability produced by a higher pH and the higher catalytic activity resulting from a higher temperature.

The coefficient of determination (R^2) value provides a measure of how much variability in the observed response values can be attributed to the experimental factors and their interactions. The R^2 values of 0.995 for NP,

0.996 for BPA, and 0.994 for TCS suggest that the fitted linear-plus interactions models can explain 99.5%, 99.6% and 99.4% respectively of the total variation. The F-values were 426.0 for NP, 622.5 for BPA and 361.3 for TCS. Those values, together with a p value of <0.001 for all eliminations, indicated that the present models are statistically significant and can predict the experimental results well.

The half-life of laccase activity was estimated to be 4 hours, 6 hours and 16 hours at a pH of 3, 4 and 5 respectively and a temperature of 40°C. The elimination of NP and BPA was directly associated with the disappearance of estrogen activity. Mass spectrometry analysis showed that the enzymatic treatment produced high molecular weight metabolites through a radical polymerization mechanism of NP, BPA and TCS.

"The design of experiments method played a critical role in this study by exploring the entire design space and helping researchers identify the optimal conditions for removal of the endocrine disrupting chemicals," Jones concluded. "This work may in the future lead to industrial-scale methods for the removal of EDCs as part of the wastewater treatment process."

For more information,
E-mail: info@statease.com,
or Peter.Jones@USherbrooke.ca.

Series 7000 mechanical diaphragm metering pumps



Neptune's Series 7000 mechanically actuated diaphragm metering pumps handle viscosities in excess of 5,000 cps and pump chemicals that off-gas (sodium hypochlorite) without binding. All models provide suction lift to 20 feet. Maximum capacities range from 15 gph to 300 gph with adjustable 10:1 turndown by micrometer dial; variable speed option allows automated flow control. Liquid ends are available in PVC, Kynar, and 316SS.

Neptune Chemical Pump Co., Inc.
Lansdale, PA
Tel: 888-3NEPTUNE or 215-699-8700
E-Mail: pump@neptune1.com
www.neptune1.com

Simply a Better Solution...



for You and the Environment

MSF

MS Filter Inc.
Water Treatment

Toll Free: 1-866-853-0164

web: www.msfilter.com